How to use DONOR™

Instructions for use for Nursing Staff

1. Close the DONOR™ system with the sliding clamp on the connecting tube.

2. Turn the vacuüm with regulator to “Off”. Disconnect tubing with Luer Lock and replace the white protection cap.

3. Connect replacement system, turn the vacuum regulator to "On" and open sliding clamp to continue wound drainage. Ensure that the green bellow is in "Max" position. note: **

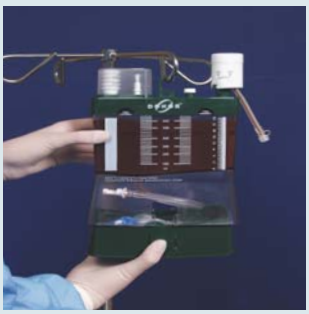

4. Release filter set by pressing the release buttons.

5. Break-off white aseptic spike entry port while holding the tubing firmly.

6. Close white tubing clamp as well as roller clamp. Ensure that the white protective cap is hanging freely.

7. Vent the DONOR™ system by snatching off the breakaway cap.

8. Remove transparent protective cap from spike and insert filter set spike firmly.

9. Prime system by opening the white tubing clamp.

10. Once blood flow into drip chamber has stopped completely, place protective cap on the air vent of the drip chamber and tighten.

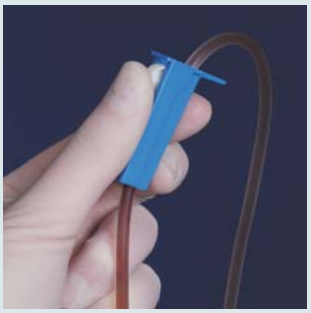

11. Open roller clamp and regulate blood flow. Ensure that the tubing has been filled completely with blood before connecting to the patient.

12. When the DONOR™ collection vessel is empty, reinfusion should be stopped by closing the roller clamp.

* These steps do not substitute the ‘Instructions for Use’ as inserted in the DONOR™ system. Read ‘Instructions for Use’ carefully before using DONOR™.

** If the replacement system is full or drainage has stopped, turn the vacuum regulator of the replacement vessel to “Off” and let the wound relax for 20 minutes before removing the drain from the wound site.

VAN STRATEN MEDICAL
PALL
MEDINORM

How to use DONOR™

Instructions for use for OR/Recovery



1. Insert and pass trocar/wound tubing into desired location until the black line indicator appears just outside skin surface. Do ensure that the section of wound tubing between the two black lines is not exposed at the surface.

2. Cut Y-drain connector to appropriate size for wound tubing.

3. With sterile scissors, cut wound tubing at a 45-degree angle for easier insertion into Y-drain connector.



4. Insert wound tubing into the Y-drain connector neck and insert fully.



5. (Optional) Attach the tubing wall suction line to the Luer-Lock connector and apply suction until exudates reaches the end of the tube but not further than the sliding clamp. Close filled tube with sliding clamp to hold wound compression.

6. Unscrew red or white protective safety cap.

7. Activate the DONOR™ system by turning the vacuum regulator to "On".

8. Open the sliding clamp to activate the DONOR™ system.

9. Close the sliding clamp when the DONOR™ system is full or drainage has stopped.